



Automotive

ManTooth™ Tethered Pressure Wireless Digital P/T Gauge



P/N 67006

Automotive

ManTooth™ Un-Tethered Pressure Wireless Digital P/T Gauge



P/N 67007

User's Manual



Made for iPhone 6 Plus, iPhone 6, iPhone 5s, iPhone 5c, iPhone 5, iPhone 4s, iPhone 4, iPad Air 2, iPad Air, iPad mini 3, iPad with Retina display, iPad (4th generation), iPad (3rd generation), iPad 2

"Made for iPhone" and "Made for iPad" mean that an electronic accessory has been designed to connect specifically to iPhone, or iPad, respectively, and has been certified by the developer to meet Apple performance standards. Apple is not responsible for the operation of this device or its compliance with safety and regulatory standards. Please note that the use of this accessory with iPhone, or iPad may affect wireless performance.



iPhone, iPad and Retina are trademarks of Apple Inc., registered in the U.S. and other countries. iPad Air and iPad mini are trademarks of Apple, Inc. Android and Google Play are trademarks of Google Inc. The Bluetooth® word mark and logos are registered trademarks owned by Bluetooth SIG, Inc. and any use of such marks by Ritchie Engineering is under license. Other trademarks and trade names are those of their respective owners.



Before You Start

Contact Ritchie Engineering Co., Inc.

To order accessories, receive assistance, or locate the nearest YELLOW JACKET distributor.

Corporate Office and Mailing Address:

Ritchie Engineering Co., Inc.
YELLOW JACKET Products Division
10950 Hampshire Avenue South
Bloomington, MN 55438-2623 USA
Phone: 952-943-1300 or 800-769-8370
Fax: 800-769-8370
Email: custserv@yellowjacket.com
www.yellowjacket.com

Safety Information

Use the instrument only as specified in this manual. Otherwise, the protection provided by the instrument may be impaired. Refer to the safety information.

A Warning identifies conditions and actions that pose hazards to the user. A Caution identifies conditions and actions that may damage the instrument or the equipment under test.

Warning

To avoid personal injury or death, follow these guidelines:

- Most governments and legal authorities require that HVAC technicians be trained and certified in the safe and proper operation of HVAC tools, such as this instrument. Since this tool may be connected to many types of equipment through a limitless combination of hoses and fittings, proper training is the most important element of using this tool safely.

- Read the entire User's Manual before using the instrument.
- Use the instrument only as described in this User's Manual, otherwise the protection provided by the equipment may be impaired.
- Do not use the instrument if it is damaged. Before you use the instrument, inspect the case. Look for cracks or loose components.
- The instrument contains no internal user serviceable parts.
- Do not open the instrument.
- Have the instrument serviced only by Ritchie Engineering Co., Inc. or authorized service centers.
- Do not use the instrument if it operates abnormally. Protection may be impaired. When in doubt, have the instrument serviced.
- Do not operate the instrument around explosive gas, vapor, or dust.
- Various refrigerants have been intentionally excluded for very significant safety reasons.
- Never use refrigerants in this instrument that are not listed in the set up menu.
- The refrigerant database in this unit may include refrigerants classified as flammable. If such refrigerants are selected, the operator may need additional certifications and/or training. Consult your government and legal authority and comply fully with all requirements.
- Always wear eye and skin protection when working with refrigerants. Escaping refrigerant vapors with present a freezing danger. Do not direct refrigerant vapors venting from hoses towards the skin.
- Maximum Working Pressure: 700 psia (4.83 MPa)
- Because this instrument allows for various inputs including electrical and mechanical, care must be taken to observe any ways that an electrical shock hazard could develop. Example: Wet or humid conditions, along with a sensor, could allow an electrical path across the instrument. Keep all interconnected equipment clean, organized, and in proper condition. Do not use the instrument if you are not qualified to recognize potential electrical faults.

Caution

To avoid damage to equipment, follow these guidelines:

- Do not allow pressures beyond the specifications listed in the manual.
- Do not attempt to introduce liquid or samples heavily laden with oil into the instrument.
- Read and observe instructions and specifications related to the batteries used in this instrument that may cause damage to it.
- Do not use this instrument on systems containing leak sealing chemicals. These leak sealants can collect and harden in the instrument, causing permanent damage.
- Only use this instrument with the protective boot in place as this protects the charging port and temperature probe connection ports from unwanted contaminants.
- Do not use damaged USB chargers to recharge the ManTooth PT Module as this could damage the circuitry and/or battery.
- Only use with refrigerants approved for use with the ManTooth PT Module. Use of unapproved refrigerants may cause damage to the ManTooth Module. A complete list of approved refrigerants can be found in the ManTooth RSA app in the “Select Refrigerant” option.

Getting Started

The ManTooth PT Module is a precise instrument to accurately measure and report the critical information needed to service refrigeration and air-conditioning equipment. The ManTooth PT Module reports the system information directly to your smartphone or tablet by means of a class 1 Bluetooth v.2.1 radio. The ManTooth PT Module is compatible with any iOS device running iOS 7.0 or later and Android devices running Android 4.0.3 (Ice Cream Sandwich) or later.

Before you use your ManTooth PT Module for the first time, you should make sure it is fully charged. You will also need to download the free ManTooth RSA Pressure/Temperature App from the Apple App Store for iOS devices or the Google Play store for Android devices.


You can either use the QR code links that are on your ManTooth PT Module packaging, follow the links that are available on www.yellowjacket.com, or just search for YELLOW JACKET ManTooth in either app store.

Pairing

To display service readings your ManTooth PT Module must be connected via Bluetooth to an iOS phone or tablet running iOS 7.0+ or an Android phone running Android 4.0.3+ (Ice Cream Sandwich or later). To connect your ManTooth PT Module to your phone or tablet the two must first be paired to one another. The pairing of the module to your device is done in your phone or tablet settings. Note - you only need to pair your ManTooth PT Module the first time you connect it to you phone or tablet; however, if you force your phone or tablet to “forget” your ManTooth PT Module, you will need to re-pair. Note - your ManTooth PT Module can be paired with multiple devices at the same time. However, it can only be connected and sending readings to one phone or tablet at a time.

To pair your ManTooth PT Module you first need to open the settings menu on the phone or tablet you wish to pair to your ManTooth PT Module. Next tap on “Bluetooth” to enter the Bluetooth settings. Be sure to turn your phone or tablet’s Bluetooth radio on if it is not already on.

Apple iOS

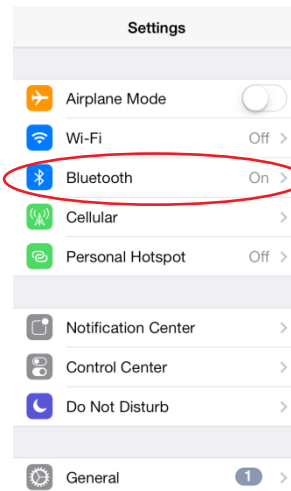


Android



Next turn your ManTooth PT Module on by pressing and releasing the power button on the main module. If you have a 67006 dual unit, the main module is the one that says, “ManTooth PT Module” on the label, not the one that says, “ManTooth PT Tether Module”. The module will go through a brief start up sequence, then the light on your ManTooth PT Module should start to blink blue. This means your ManTooth PT Module is searching for available Bluetooth devices to connect with. Next, if you are using an Android phone, tap on “Scan” at the bottom of the screen to scan for available devices. Apple iOS devices should automatically scan for available Bluetooth devices.


1. The iOS app is built specifically for the iPhone, not the iPad. If you are using an iPad and want to download the ManTooth app, you must change the tablet to iPhone only, or
2. You can directly connect to an iPhone or iPad by going to Bluetooth and turning on the ManTooth. The device will find the ManTooth PT Module and ask if you would like to download the app.

Android

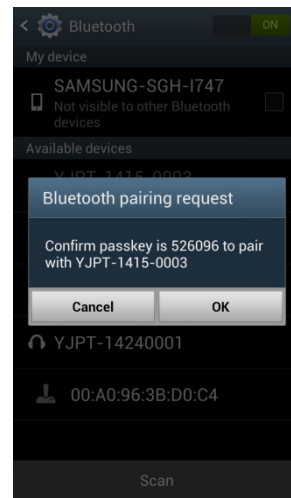


After pairing your Apple iOS phone or tablet to your ManTooth PT Module, it should show up as either “Connected” or “Not Connected” rather than “not Paired” on the Bluetooth settings screen. On Android devices under the “Paired devices” section on the Bluetooth settings screen.


Apple iOS

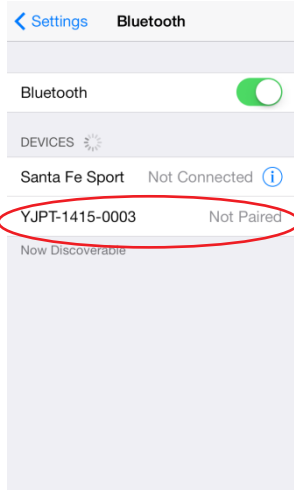


Android

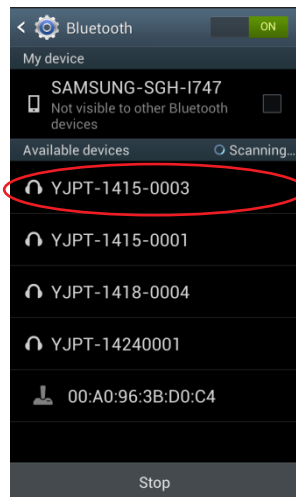

Apple iOS

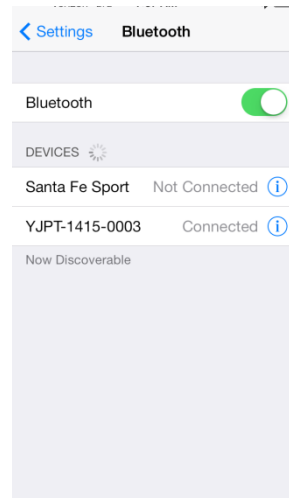

Android

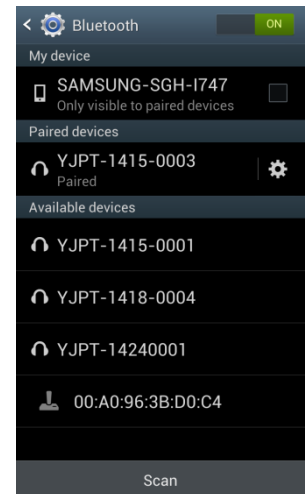


Your ManTooth PT Module should then show up as an available device to pair with on your phone or tablet’s screen. This may take up to 30 seconds.

Note: Your automotive ManTooth PT Module’s name is the same as the serial number and is printed on the main module’s label.

On Apple iOS devices once your ManTooth Module is paired if it is listed as “Connected” the light on the module will glow solid blue. However, on all Android devices or if your iOS device lists your ManTooth PT Module as “Not Connected” the light will continue to blink blue. This is normal.

ManTooth RSA App

This section will go over the various functions, settings, and procedures of the ManTooth RSA Pressure/Temperature App.


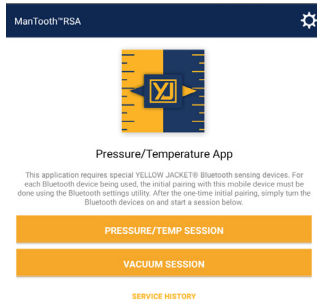


If you have not already downloaded the YELLOW JACKET ManTooth RSA Pressure/Temperature App go to either the Apple App store or the Google Play store now to download the free app. You can either use the QR code links that are on your ManTooth PT Module packaging, follow the links that are available on www.yellowjacket.com, or just search for YELLOW JACKET ManTooth in either app store.

General Settings

The General Settings menu is where you can set up and change various functions of your ManTooth RSA app to personalize it for your specific needs.

To access the general settings on the first screen available upon opening the ManTooth RSA app, tap on the gear in the upper right corner of the screen.

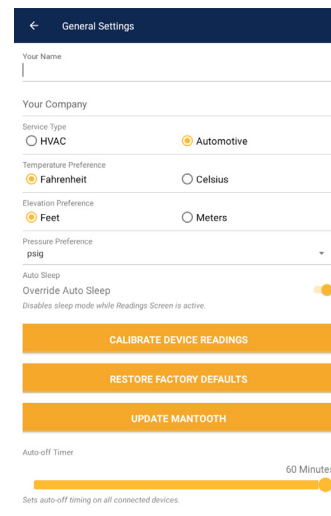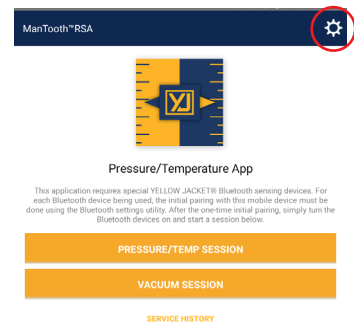

Service Management

Your Information

Here you can set your own name and your company name. This information will automatically appear in the emails containing the system readings which you can send directly from within the app.

Preferences

HVAC/Automotive

Choosing automotive will change the start screen to A/C SYSTEM CHECK and VACUUM session will disappear. The list will only contain SNAP approved refrigerants. If your ManTooth Module serial number starts with YJPT, it is for Pressure and Temperature only, it does not have vacuum capabilities. For vacuum reading in addition to pressure and temperature you will need a PTV ManTooth with a serial number starting with YJG2.

Temperature Preference

Set the units that the temperature readings from the temperature sensors, vapor saturation, liquid saturation, and the values for superheating and subcooling are displayed in. Options are degrees Fahrenheit (°F) or degrees Celsius (°C). Default temperature units are degrees Fahrenheit (°F).

Pressure Preference

Set the units that the pressure readings are displayed in. Available units are bar, pounds per square inch absolute (psia), pounds per square inch gauge (psig), kilopascals (kPa), Megapascals (MPa), and kilogram per square centimeter (kg/cm²). The default pressure units are pounds per square inch gage (psig).

Auto Sleep

This option will disable your phone or tablet's automatic sleep function so that while you are in a session taking readings your phone or tablet will not automatically go to sleep which could disrupt your session and readings. The default auto sleep setting is Override Auto Sleep = Off.

Device Management

Power Down Connected Devices

This is another way of shutting off your connected ManTooth PT Module(s) if you are not near enough to your module(s) to press the power button(s) and want to turn the power completely off.

Calibrate Device Readings

This gives you the option to adjust the calibration of your ManTooth PT Module's pressure readings or temperature readings away from the factory defaults.

Restore Factory Defaults

This will clear any calibration adjustments that have been done on the ManTooth PT Module since it left the factory.


Auto Off


This slider gives you the option of having your ManTooth PT Module automatically turn itself off after a designated period of time. It can be set anywhere from 1 to 90 minutes in iOS, 1 to 60 in Android. After the ManTooth PT Module has been connected for the specified auto off time an alert will pop up asking if you would like to reset the timer simply tap anywhere on the screen. Also included is an auto off never setting. Moving the slider all the way to the left will set the auto off timer to never. Default is Auto Off = 5 min.

Getting Back to the Previous Screen

To return to the previous screen from the one you are currently viewing, tap on the icon in the upper left hand corner. This function is the same in all of the screens in the ManTooth RSA app.


Service History

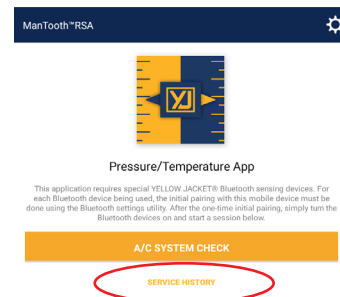

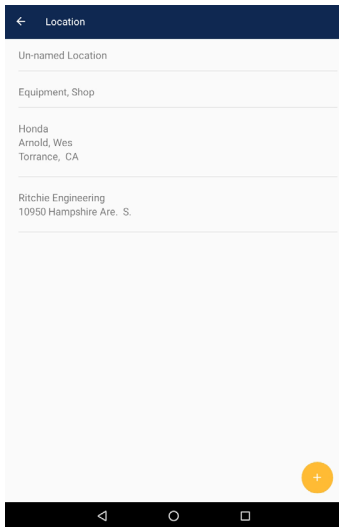


In service history you are able to browse through data that was saved during previous service sessions. Saved data is organized alphabetically by location, then by each location’s equipment, finally by date and time the data was taken. If you tap on the desired service history reading, you can see the reading that was taken and either email the reading to someone or delete it. Remember once you delete a reading, it CAN NOT be retrieved.

A/C System Check

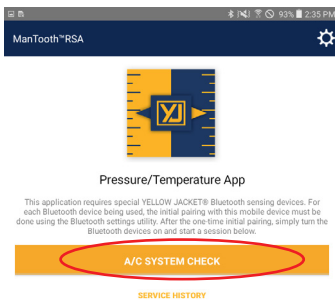

Sessions are where you connect your phone or tablet with your ManTooth PT Module to see and collect system readings. To begin a new session, tap on “A/C System Check” in the app home screen.

Session Settings

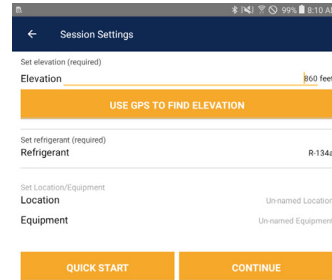

Using the correct settings that are specific for the current system you are servicing will ensure the best possible pressure readings as well as liquid and vapor saturation values.

Set Elevation

Setting the elevation will enable your ManTooth RSA app to correct for elevation pressure variations allowing for more accurate pressure readings. You may either use your phone or tablet’s built in GPS to determine your elevation or input the elevation manually by tapping on the elevation and entering your elevation above sea level in FEET. Note: “Use GPS to Find Location” functionality may not work on all devices, especially those without cellular service.

Set Refrigerant

To set the refrigerant for the current session, tap on “Refrigerant” then scroll through the list of refrigerants and select the refrigerant corresponding to the unit you will be servicing. Setting a refrigerant is mandatory before moving to the next screen.


*****WARNING*****

Refrigerants classified as flammable are in red text. If such refrigerants are selected, the operator may need additional certifications and/or training. Consult your local government and legal authority and comply fully with all requirements.

Set Location Details


If you want to organize your saved data in session history, you can enter the location information for the current service session. This information will show up in the service reports you can email and is how the service history will be organized. Here you have the ability to either add a new location or select an existing location. Once you have designated a location you can also designate what equipment is being serviced during the session., Locations can have multiple pieces of equipment associated with them so you can keep track of each individual unit at locations that may have more than one system. Saved session data will be saved to “Session History” in the app’s main menu and sorted first alphabetically by business name or customer last name, then alphabetically by assigned equipment name, and lastly by the date and time the data was saved. Note: Location details are optional . Any saved data without an assigned location will be saved under un-named location and appear at the end of the Service History list. The un-named location data will be sorted simply by date and time. You CAN NOT assign a location to data at a later time.

Assign Devices and Zero

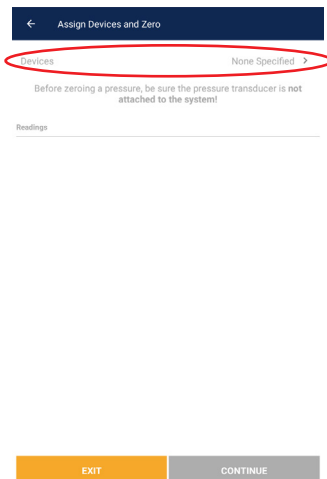


Assign Detected Devices

Now you are ready to connect your ManTooth PT Module to your current session. To connect your module first tap on “Devices None Specified”, this will take you to the next screen.



Tap on the ManTooth PT Module(s) that you wish to connect to your session from the list of devices that are displayed. Remember your module’s name is the serial number printed on the main label and should take the form of YJPT-XXXX-XXXX. Next tap the save icon in the upper right corner of the screen to save the module(s) to the session. Note: On iOS devices you must tap on “Connect a Device” to first connect your device to your phone or tablet and then select it under the “Select From Connecting Devices” heading to fully connect it to your session. Note: To connect to your ManTooth PT Module(s), your module(s) must be on and searching for a connection (where the blue light is blinking).

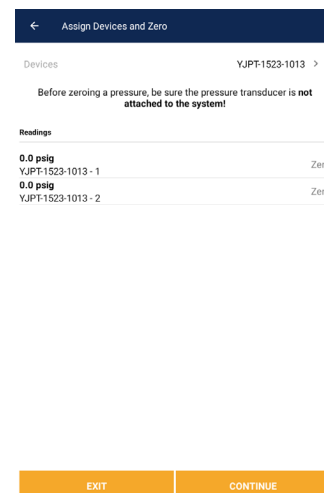


After you save your module(s) to the session, they will be displayed at the top of the screen under Assign Devices. The pressures from the connected module(s) will be displayed at the bottom of the screen. To zero the pressure transducer readings, tap on “Zero” next to the corresponding pressure.

Note: It is recommended that you zero the pressure transducer(s) at the beginning of each new session before connecting you ManTooth PT Module to the system. This will ensure the most accurate device readings.

Readings

The readings screen will display the pressures and temperatures as measured by the ManTooth PT Module, display the liquid and vapor saturation values, as well as calculate and display the superheat and subcooling values.

The first time you connect your ManTooth PT Module to a new phone or tablet you will have to assign the pressure transducers and temperature sensors. These assignments are not permanent and can be changed at anytime. **Note:** The pressure transducer in every ManTooth PT Module (main or tethered) is capable of accurately reading pressures up to 700 psia (48.3 bar) and therefore can reliably be used on either the high or low side.

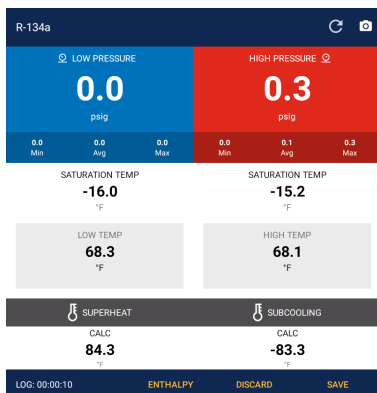

Pressure

To assign pressure readings to either the high or low side simply tap on the box that contains the value you wish to assign and select the sensor that you want to assign to that spot. **Note:** On dual units with 2 transducers the main unit is #1 and the tethered unit is #2. If you are using two single units, reference the device name/serial number to determine which pressure is associated with which device.

Pressure
0.0 psig
YJPT-1415-0003 - 1
0.0 psig
YJPT-1415-0003 - 2

Liquid and Vapor Saturation

Liquid and Vapor Saturation values are calculated automatically by the app based on the measured pressure and the refrigerant selected.

Temperature

To assign temperature readings to either the high or low side simply tap on the box that contains the value you wish to assign and select the sensor that you want to assign to that spot. **Note:** The label on the ManTooth PT Module denotes which temperature port is T1 and which is T2 for easy reference.

Subcooling and Superheat

Subcooling and Superheat are automatically calculated based on the assigned pressures and temperatures.

Enthalpy Feature Directions


The enthalpy feature will take data from four sensors, high and low pressure, and high and low temperature, and process that data through an Enthalpy Utility to generation enthalpy for the HVAC system. This data then will be applied to an App view of an enthalpy chart and will draw the appropriate polygon (or left and right side only) overlaid over the given enthalpy chart with the points lined up perfectly. This chart is a visual guide to the technician which can be used to quickly diagnose the health and energy consumption of a system connected to a ManTooth device. Note: Even though the ManTooth supports hundreds of refrigerants, this new feature only applies to R-134a and 1234yf.

Steps

1. Make sure you have two temp probes plugged into the ManTooth
2. Start an A/C SYSTEM CHECK session
3. Choose either R-134a or R1234yf refrigerants
4. Connect to the device and start the session
5. Assign all of the Pressure and Temp probes

If all of the above steps have been completed, the “ENTHALPY” button should appear at the bottom of the Readings screen. Clicking the ENTHALPY button will display the chart with real-time data and graph.



To return to the readings screen, click anywhere on the enthalpy chart.

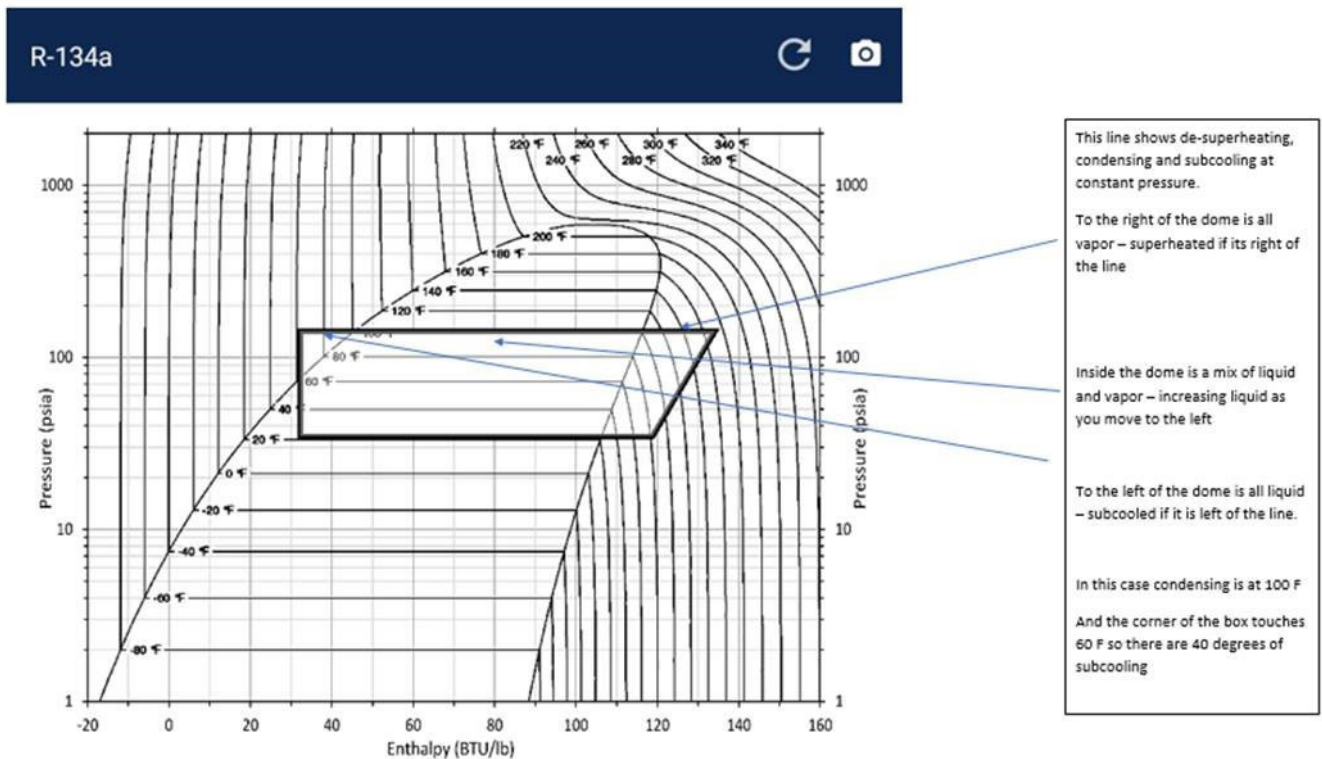

Saving Data

To save the screen shot currently on the screen, tap on the screen shot icon on the top right corner of the readings screen.

Once you choose to save the data you will be given the option to save and email, which will save it to your session history and embed the data into an email report for you to send to whoever you want, discard the snapshot you took, or just save it to your session history for later reference and use. To save the current data log at the end of a session, tap on SAVE. Once you have chosen to save the data you will be given the option to SAVE & EMAIL, which will save it to your session history and embed the data into an email report. When you tap on SAVE in iOS, it will be saved as a CSV file. Android can be saved as a CSV or a HTML file. Note: The phone or tablet you are using must be connected to cellular service or WiFi to send emails. If your phone or tablet does not have the proper service to send an email when the screen shots are taken you can save the data and then access it at any time from the “Session History” section on the app’s home screen. Any saved service data can be emailed from within “Session History”.

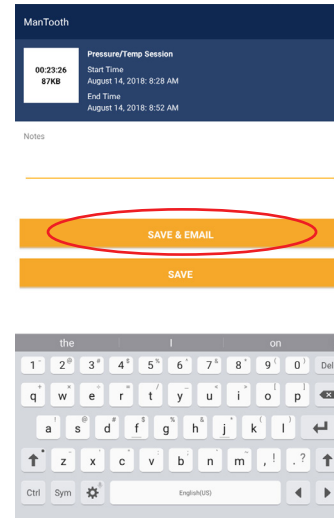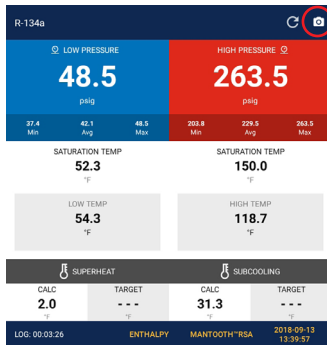

DISCARD


At the end of a session, if you don't want to save the information, tap on DISCARD. This deletes all session information and is no longer accessible.

Connection of ManTooth to a Vehicle

Prior to starting the vehicle, connect the previously zeroed ManTooth to the coupled hoses and connect the couplers to the vehicle's service ports. Make sure all ManTooth transducers, wires, and temperature clamps are clear of any moving parts (fan blades, belts, etc.) and high heat sources that could damage the components. Start the vehicle and begin your session. When the session is completed, disconnect the low side coupler from the vehicle. Waiting a couple of minutes before disconnecting the high side coupler will minimize the loss of refrigerant, oil, and dye. Next, slowly loosen the hose connections to the ManTooth transducers to relieve pressures. **WARNING:** Dye and oil may be mixed with the refrigerant. Prior to starting each session, make sure there is no residual pressure in the ManTooth units.

CAUTION: Never zero the ManTooth transducers when under pressure.

ManTooth PT Module

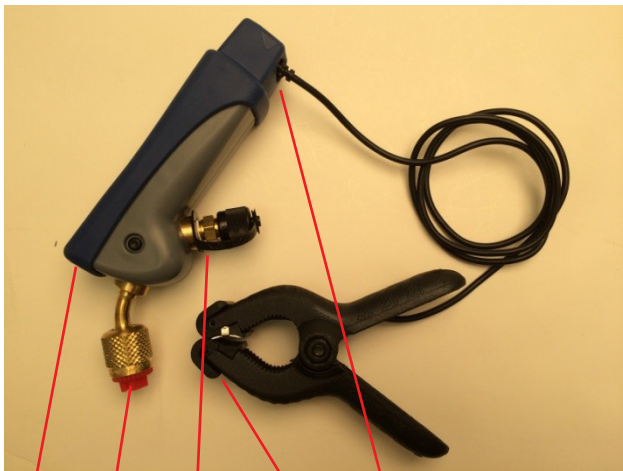

1. Status light
2. Power button
3. Device name
4. Temperature probe indicators
5. Micro USB charging port
6. 1/4" Flare fitting pressure transducer connection
7. 1/4" Flare fitting with Schrader core pressure transducer connection
8. ManTooth thermistor temperature clamp
9. Temperature probe jacks

Note: On 67006 tethered units numbers 1-4, 5, and 9 are on the main unit only. The tethered unit is only equipped with the flare fittings for measuring refrigerant pressure and adjusting charge.

Status Light

The multi-colored LED indicates the status of your ManTooth PT Module.

Blinking Blue: The module is on and searching for a Bluetooth connection. This will continue from when you turn on your ManTooth PT Module until you connect to it within the ManTooth RSA Pressure/Temperature app. **Note:** If your ManTooth PT Module loses connection to your phone or tablet it will automatically revert back to this searching for a connection mode.

Solid Blue: The module is on and connected to a phone or tablet via Bluetooth.

Solid Green: The module is connected to a power source via the Micro USB port and is charging. **Note:** Once the unit is fully charged, the green light will turn off.

Blinking Red (Short): The module will blink short flashes of red to indicate that it is sending data to a connected device. This will occur while the light is solid blue.

Blinking Red (Long): The module will flash long blinks of red when the battery level has below 10% of total life remaining.

Power Button

To turn your ManTooth PT Module on or off, push and release the power button once.

Device Name

Your ManTooth PT Module's name is displayed on the label for easy reference. The name takes the form of YJPT-XXXX-XXXX. The device name serves as your ManTooth PT Module's name within the ManTooth RSA app, its serial number, as well as its Bluetooth name that will appear on your phone or tablet when pairing.

Temperature Probe Indicator

On the label of the ManTooth PT Module T1 and T2 are printed onto the label to indicate which temperature port on the back of the device corresponds to temperature port 1 (T1) and temperature port 2 (T2).

Micro USB Charging Port

The ManTooth PT Module is designed to be charged using any standard Micro USB charging cord and corresponding USB charger.

1/4" Flare Fitting Pressure Transducer Connection

The flare fitting on the front of the ManTooth PT Module directs to the pressure transducer with a working pressure range of 0-700 psia. The fitting is equipped with an "Adjust-a-Valve" opener and sized to fit most system access ports for easy access to most AC and refrigeration units. The compact size of the ManTooth PT Module and short hose connection system reduces charging loss that can occur from hoses used in charging through a standard test and charge manifold. Adapters to connect the ManTooth PT Module to other size access ports are available from YELLOW JACKET.

1/4" Flare Fitting with Schrader Core Pressure Transducer Connection

The Schrader core fitting on the ManTooth PT Module allows for recovering refrigerant, adding charge, or removing charge all without disconnecting your ManTooth PT Module from the system.

ManTooth Thermistor Clamp

The thermistor pipe clamp probe is capable of clamping to and measuring the temperature of pipes ranging in size from 1/4" to 1 3/8". The probe is capable of measuring with an accuracy of 0.2°C from 0°C to 70°C with a full range of -40°C to 130°C. For best long term stability of your thermistor pipe clamp probe, avoid storing it at temperatures exceeding 75°C (167°F).

Thermistor Probe Jacks

Each ManTooth PT Module is equipped with 2 temperature probe jacks for use with ManTooth Thermistor Clamps.

Instrumentation Specification

Pressure Sensing Resolution	0.1 psi, 0.1 bar, 1 kPa, 0.01 MPa, 0.01 kg/cm ²
Pressure Sensing Accuracy	0.5% of full scale at 25°C 1% of full scale 55°F to 130°F 2% of full scale -40°F to 248°F
Working Pressure	0 to 700 psia (48.3 bar)
Proof Pressure	Tolerable pressure without loss of seal 1500 psia

Burst Pressure	Tolerable pressure without internal damage 1000 psia
Temperature Sensor Range (instrument)	Sensing element -40°F to 266°F (-40°C to 130°C) Max cord temp 203°F (95°C)
Temperature Display Resolution	0.1°F or °C
Temperature Accuracy (instrument)	± 0.2 °C (±0.36°F)
Working Temperature	-4°F to 160°F For best battery performance do not store at over 100°F
Working Humidity	0-95% RH (non-condensing)
IP Class	IP 50
Battery Life	10+ hours continuous
Range	Up to 400 feet Limited by phone or tablet Bluetooth radio strength Note: As with any radio technology, when you start to add obstructions between the transmitter and the receiver, the ultimate range may decrease as different objects interfere with the radio signal in different ways. The more obstructions you add between the phone and the ManTooth, the weaker the signal may become after it has passed through or around the obstacles. This could ultimately lead to a shorter maximum range. The ManTooth utilized the highest Bluetooth radio transmitter signal strength available to ensure the best possible range of your ManTooth; however, each situation will be slightly different depending on the environment/surroundings within you are working.
Bluetooth Radio	Class 1 Bluetooth 2.1 Radio
Size	6" long x 1.6" wide x 2.3" thick (15.3 x 4 x 5.8cm)
Weight	0.5 lbs (225 g)
Superheat and Subcool	Automatically calculated by the ManTooth app

Warranty Policy

The **YELLOW JACKET ManTooth Wireless Digital PT Gauge** from Ritchie Engineering Co, Inc. is guaranteed to be free from material and workmanship defects for a period of two years. All other **YELLOW JACKET** products included in this package are guaranteed to be free from material and workmanship defects for a period of one year. These guarantees do not cover products that have been altered, abused, misused, or improperly maintained.

Not all cataloged products are stocked and eligible for return. Please check with your **YELLOW JACKET** representative of the factory for more information.

All returns must have an RGA number and proof of purchase/copy of invoice. Please obtain an RGA number from Ritchie Engineering Customer Service by calling 800-769-8370.

All returns must be pre-paid.

Max. and Min. Pressures	Displays and records the maximum and minimum pressures
Refrigerant Database	All SNAP refrigerant profiles included; upgradeable
Share Screen Shots	Screen shot feature allows you to save pressure and temperature readings from your sessions which can be automatically organized by location and unit being serviced.
Temperature Sensors	Capable of measuring two temperatures using high accuracy NTC thermistors
Pressure Transducers	67006 - Two tethered pressure transducers 67007 - Two individual pressure transducers
System Attachment	Very small internal volume minimized refrigerant loss during system analysis. Standard manifolds and hoses can lose over 50 times more refrigerant with each connection
Pressure Zeroing	Simple single button zeroing at the start of each session
Elevation Compensation	Enter elevation at the start of the session for effortless psia compensation
Battery	Rechargeable LiPo battery for long battery life and excellent recharging capability for the life of your ManTooth

UPC #	Description
67006	ManTooth (two singles tethered) Automotive Kit: hi- and lo-side hoses, R-134a and R-1234YF couplers, temperature clamps, USB cord and charger, and case
67007	ManTooth (two singles un-tethered) Automotive Kit: hi- and lo-side hoses, R-134a and R-1234YF couplers, temperature clamps, USB cord and charger, and case
UPC #	Replacement Parts
67036	Red hose R-134a
67037	Blue hose R-134a
67038	Red hose R-1234YF
67039	Blue hose R-1234YF
41337	Hi-side R-134a coupler
41338	Lo-side R-134a coupler
41441	Hi-side R-1234YF coupler
41442	Lo-side R-1234YF coupler
93394	Tether cap
19020	Hose gaskets (10 pak)
67012	USB cord
67018	Carrying case



Ritchie Engineering Co., Inc.
YELLOW JACKET Products Division
 10950 Hampshire Avenue South
 Bloomington, MN 55438 USA

Phone: 800-769-8370
 952-943-1300

Fax: 800-322-8684

Email: custserv@yellowjacket.com
www.yellowjacket.com

©2018 Ritchie Engineering Co., Inc.